(54) Title: A RATE ADAPTIVE PACEMAKER
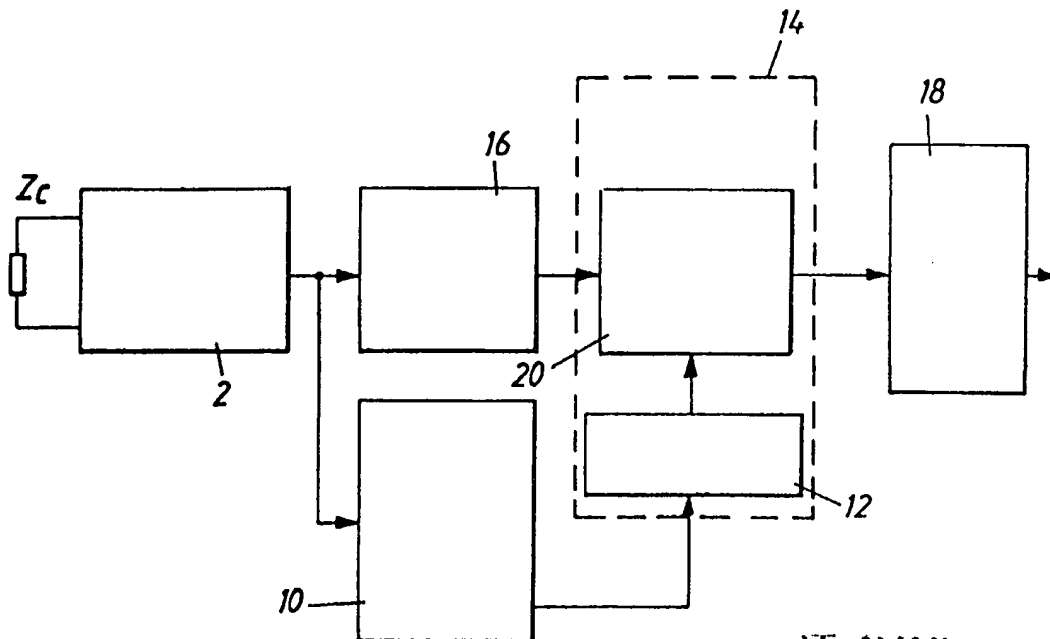
(57) Abstract

A rate adaptive pacemaker comprises a means (2) for determining the demand of the patient's organism, a pacing rate controlling means (16) for controlling the pacing rate in response to the patient's demand, and a pacing rate limiting means (20) for preventing the pacing rate from becoming too low. The pacing rate limiting means is adapted to limit the pacing rate downwards such that a first predetermined relation is satisfied between actual cardiac output (CO) and cardiac output (CO_{rest}) for the patient in rest conditions and a second predetermined relation is satisfied between actual stroke volume (SV) and rest stroke volume (SV_{rest}).

A RATE ADAPTIVE PACEMAKER

Technical Field

The present invention relates to a rate adaptive pacemaker comprising a means for determining the demand of the patient's organism, a pacing rate controlling means for controlling the pacing rate in response to the patient's demand, and a pacing rate limiting means for preventing the pacing rate from becoming too low.

Background Art

The pacing rate of a rate adaptive pacemaker may become too low due to the physical demand of the patient's organism and heart. This may result in lack of oxygen supply to the myocardium. Under certain conditions the heart may not be able to fulfil the physiological needs of the patient's organism and heart if the pacing rate is not limited.

It is previously known to set a lower limit for the pacing rate. This limit value is normally determined from the patient's diagnosis and a constant or externally programmable limit can be set. Thus US-A-4,535,774 describes a stroke volume controlled pacemaker, in which the heart rate is permitted to range between prescribed minimum and maximum heart rate values. Further, in US-A-5,861,011 a pacemaker is disclosed having a system for determining the circadian rhythm by examining variations in the QT interval and adjusting the pacemaker night time setting of a lower rate limit to a lower value than the pacemaker daytime setting of the lower rate limit.

Thus, too low a pacing rate may cause too slow influx of blood enriched with oxygen. A prescribed suitable lower pacing rate limit avoids the slow influx of the fresh blood. At the same time this lower limit value should be low enough not to disturb a peaceful sleep. In that case the patient can feel more healthy in various everyday life conditions including peaceful sleeping.

2

The purpose of the present invention is to provide a rate adaptive pacemaker in which the pacing rate is prevented in a new way from becoming too low, such that the above discussed

5   inconveniences for the patient are avoided.

Disclosure of the Invention

This purpose is obtained by a rate adaptive pacemaker according to claim 1.

10

Thus, by satisfying two predetermined relations the pacemaker according to the invention ensures a sufficient minimum energy supply to the patient's organism or body and at the same time the maximum value of the stroke volume is limited

15   and these conditions are continuously automatically checked.

Preferred embodiments are set forth in the dependent claims.

According to an advantageous embodiment of the pacemaker

20   according to the invention the first predetermined relation is

$$CO > CO_{rest} \qquad\qquad (1)$$

and said second predetermined relation is

$$(SV)/(SV_{rest}) < L \qquad\qquad (2)$$

25   where L denotes a predetermined constant > 1, preferably equal to a value between 1.2 and 1.5. In this way the actual cardiac output is ensured not to become lower than the rest state cardiac output CO_{rest} and the actual stroke volume is ensured to be less than a maximum allowed value equal to $L \times$

30   SV_{rest}, where L typically has a value between 1.2 and 1.5, depending on the health of the patient's myocardium. By satisfying both these conditions simultaneously a physio-logically well founded heart work management at low work loads is ensured.

35

According to other advantageous embodiments of the pacemaker according to the invention the pacing rate limiting means includes a lower limit setting means for setting a lower limit value for the pacing rate, and a lower limit determin-
5   ing means for determining the relation between actual cardiac output (CO) and cardiac output (CO_{rest}) for the patent in rest conditions, and the relation between actual stroke volume (SV) and a rest stroke volume (SV_{rest}) and calculating a lower pacing rate limit value from said relations for supply to
10   said limit setting means, and said lower limit determining means includes a stroke volume measuring means for measuring actual stroke volume SV and comparison means for comparing measured actual stroke volume SV with stroke volume SV_{rest} for the patient in rest conditions to ensure that the inequality

15                                    $$SV/SV_{rest} < L \qquad\qquad (3)$$

is satisfied and said lower limit determining means is adapted to calculate a lower pacing rate limit value from the equation

$$\text{lower pacing rate limit} = HR_{rest} \cdot (SV_{rest}/SV) \qquad (4)$$

20   where HR_{rest} denotes the heart rate for the patient in rest conditions, provided that said inequality is satisfied. In this way the lower pacing rate limit is continuously auto-matically calculated and it may also happen that the lower pacing rate limit becomes lower than the typical heart rate
25   HR_{rest} for rest conditions of the patient.

According to still another advantageous embodiment of the pacemaker according to the invention a bioimpedance measure-ment unit is provided to measure the cardiac bioimpedance as
30   a function of time for determining therefrom actual cardiac output CO and actual stroke volume SV from the measured cardiac bioimpedance. In this way these parameters are obtained in an easy and reliable way from the time variation of the bioimpedance measured between a standard intracardiac

electrode and the housing of the pacemaker, when an excit-
ation current proceeds from the electrode tip.

Brief Description of the Drawings

The invention will now be described more in detail with
reference to the enclosed drawings on which figure 1 is a
block diagram of an embodiment chosen as an example of the
pacemaker according to the invention and figure 2 illustrates
the principle of bioimpedance measurements between the tip of
an intracardial electrode and the metal housing of the
pacemaker.

Description of a Preferred Embodiment

To avoid that the current cardiac output CO

$$CO = SV \times HR \qquad (5)$$

becomes lower than the rest state cardiac output CO_{rest} the
pacing rate must be above a lower pacing rate limit given by

$$\text{lower pacing rate limit} = (CO_{rest})/(SV) \qquad (6)$$

and since

$$CO_{rest} = HR_{rest} \times SV_{rest} \qquad (7)$$

$$\text{lower pacing rate limit} = (HR_{rest}) \times (SV_{rest}/SV) \qquad (8)$$

In addition thereto the maximum value of the stroke volume
must be limited, i.e.

$$SV < L \times SV_{rest} \qquad (9)$$

Thus, the following two conditions must be fulfilled
simultaneously for insuring a physiologically well founded
heart work management at low work loads.

$$\text{Pacing rate limit} > (HR_{rest}) \times (SV_{rest}/SV) \qquad (10)$$

$$SV/SV_{rest} < L \qquad (11)$$

where L is a constant typically equal to a value of 1.2 to
1.5, depending on the health of the patient's myocardium.

Thus the lower pacing rate limit is continuously auto-
matically calculated from the measured actual stroke volume
SV and known values of SV_{rest}, HR_{rest} and the constant L. The
actual stroke volume can be determined from e.g. bioimpedance
measurements as will be described below.

Figure 1 is a block diagram of an embodiment of the pacemaker
according to the invention comprising a bioimpedance measure-
ment unit 2 for measuring the time variation of the electric
intracardiac bioimpedance $Z_c(t)$. This type of measurements is
well known, see e.g. "Design of Cardiac Pacemakers", edited
by John G. Webster, IEEE Press, 1995, pp. 380-386 and US-A-
5,154,171, 5,280,429, 5,282,840 and 5,807,272. Thus the time
variation of the intracardiac bioimpedance can be measured
between the tip 4 of the intracardiac electrode 6 and the
housing 8 of the pacemaker, when an excitation current is fed
from the electrode tip 4, as schematically illustrated in
figure 2. Thus a standard pacing lead can be used for this
measurement.

From the measured time variations $\Delta Z_c(t)$ the stroke volume SV
needed for calculating the lower pacing rate limit according
to equation (8) above, or for checking the inequalities (10)
or (11), are determined in computing means 10, see figure 1.

The calculated lower limit value is supplied to a lower limit
setting means 12 of a pacing rate limiter 14.

A pacing rate controller 16 is also provided for controlling
the pacing rate of the pacer or pulse generator 18 in
response to the patient's demands. In a limiting unit 20 of
the limiter 14 the demanded pacing rate is compared to the
set lower limit pacing rate and the actual pacing rate is
limited to the set lower limit value if the demanded pacing

rate reaches this limit value. Thus in the pacemaker according to the invention a lower limit value for the pacing rate is continuously automatically determined and it is continuously automatically verified that the actual pacing rate does not exceed the present lower limit value.

Alternatively, the pacemaker can be modified to continuously monitor that the inequalities (10) or (11) above are satisfied.

Above bioimpedance measurements are described for determining the stroke volume SV. This parameter can, however, also be determined by other techniques, like by ECG measurements, by ultrasound technique, by radiometric and optical techniques etc. Generally all dynamic distance and/or capacity measuring methods are applicable.

Claims

1.   A rate adaptive pacemaker comprising a means for
determining the demand of the patient's organism, a pacing
5   rate controlling means for controlling the pacing rate in
response to the patient's demand, and a pacing rate limiting
means for preventing the pacing rate from becoming too low,
characterized in that said pacing rate limiting means is
adapted to limit the pacing rate downwards such that a first
10   predetermined relation is satisfied between actual cardiac
output (CO) and cardiac output (CO_{rest}) for the patient in
rest conditions and a second predetermined relation is
satisfied between actual stroke volume (SV) and rest stroke
volume (SV_{rest}).

15   2.   The pacemaker according to claim 1, **characterized in**
that said first predetermined relation is

$$CO > CO_{rest}$$

and said second predetermined relation is

$$(SV)/(SV_{rest}) < L$$

20   where L denotes a predetermined constant > 1, preferably
equal to a value between 1.2 and 1.5.

3.   The pacemaker according to claims 1 or 2,
characterized in that said pacing rate limiting means
includes a lower limit setting means for setting a lower
25   limit value for the pacing rate, and a lower limit
determining means for determining the relation between actual
cardiac output (CO) and cardiac output (CO_{rest}) for the
patient in rest conditions and the relation between actual
stroke volume (SV) and a rest stroke volume (SV_{rest}) and
30   calculating a lower pacing rate limit value from said
relations for supply to said limit setting means.

4.   The pacemaker according to claim 3, **characterized in**
that said lower limit determining means includes a stroke
volume measuring means for measuring actual stroke volume SV
35   and comparison means for comparing measured actual stroke
volume SV with stroke volume SV_{rest} for the patient in rest
conditions to ensure that the inequality

$$SV/SV_{rest} < L$$

is satisfied, and in that said lower limit determining means is adapted to calculate a lower pacing rate limit value from the equation

$$\text{lower pacing rate limit} = HR_{rest} \cdot (SV_{rest}/SV)$$

where HR_{rest} denotes the heart rate for the patient in rest conditions, provided that said inequality is satisfied.

5.   The pacemaker according to any of the claims 2 - 4, **characterized in** that a bioimpedance measurement unit is provided to measure the cardiac bioimpedance as a function of time for determining therefrom actual cardiac output (CO) and actual stroke volume (SV) from the measured cardiac bioimpedance.

6.   The pacemaker according to any of the claims 2 - 4, **characterized in** that an ECG measuring and analyzing unit is provided to measure ECG and determine therefrom actual cardiac output (CO) and actual stroke volume (SV).

7.   The pacemaker according to any one of claims 1 - 4, **characterized in that** a dynamic distance measuring and analyzing unit is provided to determine therefrom actual cardiac output (CO) and actual stroke volume (SV).

Fig.1
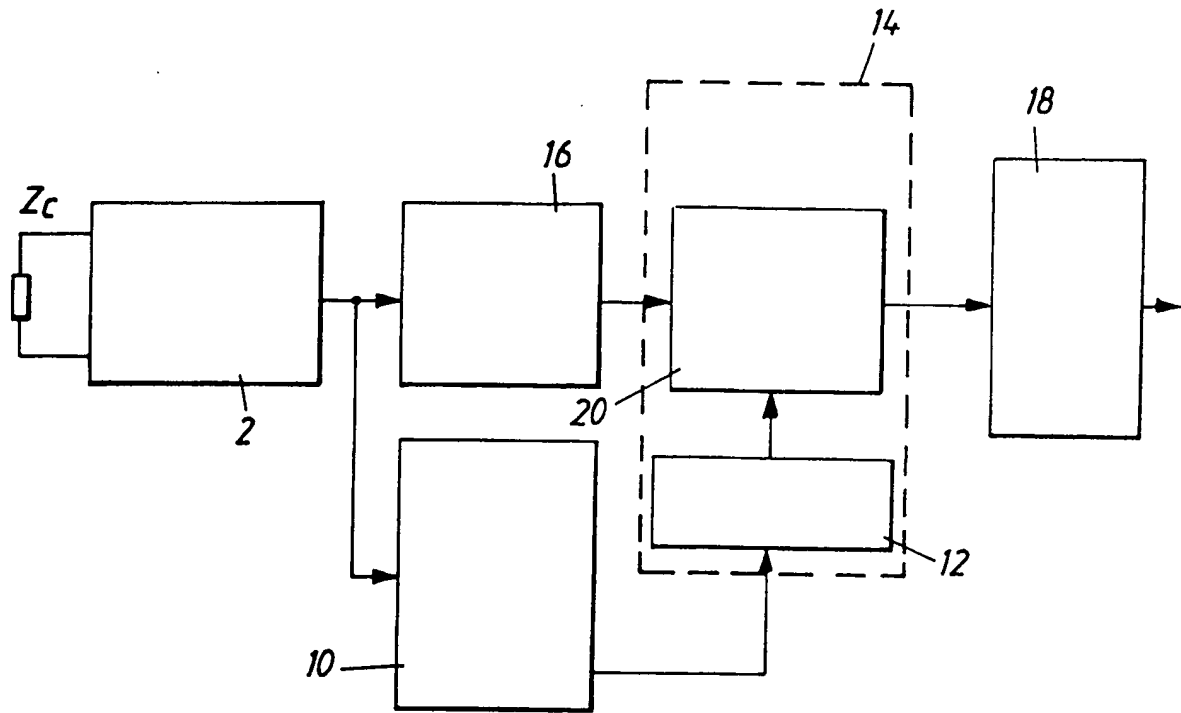
Fig. 2
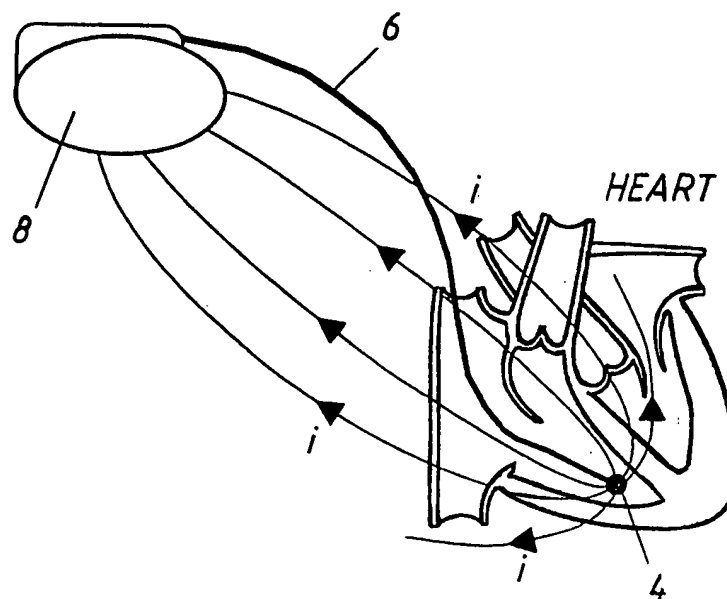
INTERNATIONAL SEARCH REPORT

International application No.

PCT/SE 00/00572

A. CLASSIFICATION OF SUBJECT MATTER

IPC7: A61N 1/365

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

IPC7: A61N

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched

SE,DK,FI,NO classes as above

Electronic data base consulted during the international search (name of data base and, where practicable, search terms used)

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
A	EP 0140472 A1 (MEDTRONIC, INC.), 8 May 1985 (08.05.85), page 11, line 7 - page 13, line 30 --	1-6
A	US 5183040 A (TIBOR A. NAPPHOLZ ET AL), 2 February 1993 (02.02.93), column 19, line 62 - column 20, line 3 --	1-6
A	EP 0576114 A2 (TELECTRONICS N.V.), 29 December 1993 (29.12.93), column 29, line 23 - line 54 -- --------	1-6

☐ Further documents are listed in the continuation of Box C. · ☒ See patent family annex.

*	Special categories of cited documents:	"T"	later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
"A"	document defining the general state of the art which is not considered to be of particular relevance		
"E"	earlier document but published on or after the international filing date	"X"	document of particular relevance: the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
"L"	document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)		
"O"	document referring to an oral disclosure, use, exhibition or other means	"Y"	document of particular relevance: the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
"P"	document published prior to the international filing date but later than the priority date claimed	"&"	document member of the same patent family

Date of the actual completion of the international search	Date of mailing of the international search report
26 June 2000	2000 -07- 2 4

Name and mailing address of the ISA/	Authorized officer
Swedish Patent Office Box 5055, S-102 42 STOCKHOLM Facsimile No. + 46 8 666 02 86	Nikolaj Hautaviita/Els Telephone No. + 46 8 782 25 00

Form PCT/ISA/210 (second sheet) (July 1992)

Patent document cited in search report			Publication date	Patent family member(s)			Publication date
EP	0140472	A1	08/05/85	CA	1243361	A	18/10/88
				JP	1701308	C	14/10/92
				JP	3068708	B	29/10/91
				JP	60034462	A	22/02/85
				US	4535774	A	20/08/85
US	5183040	A	02/02/93	NONE			
EP	0576114	A2	29/12/93	DE	576114	T	28/07/94
				US	5197467	A	30/03/93